



# **CE-EMC TEST REPORT**

for

**Product: MULTI-FIELD EMF METER**

**Model: HT627**

**Report No.: PTC23071004802E-EM01**

Issued for

**Dongguan Habotest Instrument Technology Co., Ltd.  
No.8, 4th Qinghu Xingye Road, Qingxi Town, Dongguan City, Guangdong  
Province, China**

Issued by

**Precise Testing & Certification (Guangdong) Co., Ltd.  
Building 1, No. 6, Tongxin Road, Dongcheng Street, Dongguan, Guangdong,  
China.**

**TEL: +86-769-3880 8222**

**FAX: +86-769-3882 6111**

Note: This report shall not be reproduced except in full, without the written approval of Precise Testing & Certification (Guangdong) Co., Ltd. This document may be altered or revised by Precise Testing & Certification (Guangdong) Co., Ltd. personnel only, and shall be noted in the revision section of the document. The test results presented in this report only relate to the tested sample.





## TABLE OF CONTENTS

|                                                                  |           |
|------------------------------------------------------------------|-----------|
| <b>1. TEST CERTIFICATION .....</b>                               | <b>3</b>  |
| <b>2. TEST SUMMARY .....</b>                                     | <b>4</b>  |
| <b>3. TEST SITE .....</b>                                        | <b>5</b>  |
| 3.1. TEST FACILITY .....                                         | 5         |
| 3.2. MEASUREMENT UNCERTAINTY .....                               | 5         |
| 3.3. LIST OF TEST AND MEASUREMENT INSTRUMENTS .....              | 6         |
| <b>4. EUT DESCRIPTION .....</b>                                  | <b>10</b> |
| <b>5. TEST METHODOLOGY .....</b>                                 | <b>11</b> |
| 5.1. TEST MODE .....                                             | 11        |
| 5.2. EUT SYSTEM OPERATION .....                                  | 11        |
| <b>6. SETUP OF EQUIPMENT UNDER TEST .....</b>                    | <b>12</b> |
| 6.1. DESCRIPTION OF SUPPORT UNITS .....                          | 12        |
| 6.2. CONFIGURATION OF SYSTEM UNDER TEST .....                    | 12        |
| <b>7. EMISSION TEST .....</b>                                    | <b>13</b> |
| 7.1. CONDUCTED EMISSION MEASUREMENT .....                        | 13        |
| 7.2. RADIATED EMISSION MEASUREMENT .....                         | 15        |
| 7.3. HARMONICS CURRENT MEASUREMENT .....                         | 19        |
| 7.4. VOLTAGE FLUCTUATION AND FLICKS MEASUREMENT .....            | 22        |
| <b>8. IMMUNITY TEST .....</b>                                    | <b>23</b> |
| 8.1. GENERAL DESCRIPTION .....                                   | 23        |
| 8.2. GENERAL PERFORMANCE CRITERIA DESCRIPTION .....              | 26        |
| 8.3. ELECTROSTATIC DISCHARGE (ESD) .....                         | 27        |
| 8.4. RADIATED, RADIO-FREQUENCY, ELECTROMAGNETIC FIELD (RS) ..... | 31        |
| 8.5. ELECTRICAL FAST TRANSIENT (EFT) .....                       | 34        |
| 8.6. SURGE IMMUNITY TEST .....                                   | 36        |
| 8.7. CONDUCTED RADIO FREQUENCY DISTURBANCES (CS) .....           | 38        |
| 8.8. POWER FREQUENCY MAGNETIC FIELD .....                        | 40        |
| 8.9. VOLTAGE DIP & VOLTAGE INTERRUPTIONS .....                   | 42        |
| <b>9. PHOTOGRAPHS OF THE TEST CONFIGURATION .....</b>            | <b>45</b> |
| <b>10. PHOTOGRAPHS OF EUT .....</b>                              | <b>46</b> |



Report No.: PTC23071004802E-EM01

## 1. TEST CERTIFICATION

|                       |                                                                                                                                                |
|-----------------------|------------------------------------------------------------------------------------------------------------------------------------------------|
| Product:              | MULTI-FIELD EMF METER                                                                                                                          |
| Model:                | HT627                                                                                                                                          |
| Applicant :           | Dongguan Habotest Instrument Technology Co., Ltd.                                                                                              |
| Address:              | No.8, 4th Qinghu Xingye Road, Qingxi Town, Dongguan City, Guangdong Province, China                                                            |
| Manufacturer:         | Dongguan Habotest Instrument Technology Co., Ltd.                                                                                              |
| Address:              | No.8, 4th Qinghu Xingye Road, Qingxi Town, Dongguan City, Guangdong Province, China                                                            |
| Test Date:            | July 10, 2023 to July 18, 2023                                                                                                                 |
| Issued Date:          | July 18, 2023                                                                                                                                  |
| Test Voltage:         | Battery                                                                                                                                        |
| Applicable Standards: | EMC Directive 2014/30/EU<br>EN IEC 61326-1:2021<br>EN IEC 61326-2-2:2021<br>EN IEC 61000-3-2:2019+A1:2021<br>EN 61000-3-3:2013+A1:2019+A2:2021 |

The above equipment has been tested by Precise Testing & Certification (Guangdong) Co., Ltd. and found compliance with the requirements in the technical standards mentioned above. The test results presented in this report only relate to the product/system tested. The Other similar equipment will not necessarily produce the same results due to production tolerance and measurement uncertainties.

Test Engineer.

Technical Manager.



Simon Pu /Manager



## 2. TEST SUMMARY

| EMISSION                                 |                                    |        |                    |
|------------------------------------------|------------------------------------|--------|--------------------|
| Standard                                 | Item                               | Result | Remarks            |
| CISPR<br>11:2015+A1:2016+A2:2019         | Conducted emission<br>(Mains Port) | N/A    | N/A                |
|                                          | Radiated emission                  | PASS   | Meet Class B limit |
| EN IEC<br>61000-3-2:2019+A1:2021         | Harmonic current<br>emissions      | N/A    | N/A                |
| EN<br>61000-3-3:2013+A1:2019<br>+A2:2021 | Voltage fluctuations &<br>flicker  | N/A    | N/A                |

| IMMUNITY                               |                                         |        |                                |
|----------------------------------------|-----------------------------------------|--------|--------------------------------|
| Standard                               | Item                                    | Result | Remarks                        |
| IEC 61000-4-2:2008                     | ESD                                     | PASS   | Complied with the requirements |
| IEC 61000-4-3:2006+<br>A1:2007+A2:2010 | RS                                      | PASS   | Complied with the requirements |
| IEC 61000-4-4:2012                     | EFT                                     | N/A    | N/A                            |
| IEC<br>61000-4-5:2014+A1:2017          | Surge                                   | N/A    | N/A                            |
| IEC 61000-4-6:2013                     | CS                                      | N/A    | N/A                            |
| IEC 61000-4-8:2009                     | PFMF                                    | N/A    | N/A                            |
| IEC 61000-4-11:2020                    | Voltage dips<br>& voltage<br>variations | N/A    | N/A                            |

Note: 1) The test result verdict is decided by the limit of test standard.

2) The information of measurement uncertainty is available upon the customer's request.



### 3. TEST SITE

#### 3.1. TEST FACILITY

Precise Testing & Certification (Guangdong) Co., Ltd.

Address: Building 1, No. 6, Tongxin Road, Dongcheng Street, Dongguan, Guangdong, China.

☆ CNAS Registration No.: CNAS L5772

☆ FCC Registration No.: 790290

☆ A2LA Certificate No.: 4408.01

☆ IC Registration No.: 12191A

Test Lab: Guangdong Dongguan Quality Supervision Testing Center

Address: No. 2, Industrial South Road, Songshan Lake Science and Technology Industrial Park, Dongguan City, China

Test items: radio frequency electromagnetic field immunity (R/S) test

#### 3.2. MEASUREMENT UNCERTAINTY

| Parameter                        | Uncertainty              |
|----------------------------------|--------------------------|
| Temperature                      | $\pm 1^{\circ} \text{C}$ |
| Humidity                         | $\pm 5\%$                |
| DC and Low Frequency Voltages    | $\pm 3\%$                |
| Conducted Emission(150KHz-30MHz) | $\pm 3.60\text{dB}$      |
| Radiated Emission(30MHz-1GHz)    | $\pm 4.76\text{dB}$      |
| Radiated Emission (1GHz-18GHz)   | $\pm 4.44\text{dB}$      |

Note 1: This uncertainty represents an expanded uncertainty expressed at approximately the 95% confidence level using a coverage factor of  $k=2$ .



### 3.3. LIST OF TEST AND MEASUREMENT INSTRUMENTS

#### 3.3.1. For conducted emission at the mains terminals test

| Name of Equipment        | Manufacturer  | Model           | Serial No. | Calibration Due |
|--------------------------|---------------|-----------------|------------|-----------------|
| EMI Test Receiver        | Rohde&Schwarz | ESCI            | 101417     | Aug 21, 2023    |
| Artificial Mains Network | Rohde&Schwarz | BS ENV216       | 102453     | Aug 21, 2023    |
| ISN                      | SCHWARZBECK   | NTFM8131        | 00257      | Aug 21, 2023    |
| Test S/W                 | Tonscend      | JS32-CE/4.0.0.3 |            |                 |

#### 3.3.2. For radiated emission test (30MHz-1GHz)

| Name of Equipment            | Manufacturer  | Model           | Serial No. | Calibration Due |
|------------------------------|---------------|-----------------|------------|-----------------|
| EMI Test Receiver            | Rohde&Schwarz | ESCI            | 101417     | Aug 21, 2023    |
| Bilog Antenna                | SCHWARZBECK   | VULB 9160       | 9160-3355  | Aug 21, 2023    |
| Preamplifier (low frequency) | SCHWARZBECK   | BBV 9745        | 9745-0013  | Aug 21, 2023    |
| Test S/W                     | Tonscend      | JS32-RE/4.0.0.0 |            |                 |

#### 3.3.3. For radiated emission test (1GHz above)

| Name of Equipment    | Manufacturer  | Model           | Serial No. | Calibration Due |
|----------------------|---------------|-----------------|------------|-----------------|
| EMI Test Receiver    | Rohde&Schwarz | ESCI            | 101417     | Aug 21, 2023    |
| Spectrum Analyzer    | Agilent       | E4407B          | MY45109572 | Aug 21, 2023    |
| Horn Antenna         | SCHWARZBECK   | 9120D           | 9120D-1246 | Aug 21, 2023    |
| High NOISE AMPLIFIER | ZHINAN        | ZN3380C         | 15002      | Aug 21, 2023    |
| Test S/W             | Tonscend      | JS32-RE/4.0.0.0 |            |                 |

**3.3.4. For harmonic current emissions and voltage fluctuations/flicker test**

| Name of Equipment               | Manufacturer           | Model          | Serial No. | Calibration Due |
|---------------------------------|------------------------|----------------|------------|-----------------|
| Harmonics / Flicker Test System | California Instruments | CTS/PACS-1-115 | 1534A00401 | Aug 21, 2023    |
| AC Power Source                 | California Instruments | 3001IX-208-CTS | 1534A00401 | Aug 21, 2023    |
| Test S/W                        | AMETEK                 | CTS 4          |            |                 |

**3.3.5. For electrostatic discharge immunity test**

| Name of Equipment | Manufacturer | Model   | Serial No. | Calibration Due |
|-------------------|--------------|---------|------------|-----------------|
| ESD Generator     | SCHLODER     | SESD216 | 606137     | Aug 21, 2023    |

**3.3.6. For radio frequency electromagnetic field immunity (R/S) test**

| Name of Equipment     | Manufacturer | Model             | Serial No. | Calibration Due |
|-----------------------|--------------|-------------------|------------|-----------------|
| Power meter           | Agilent      | E4419B            | GB42421440 | Aug 21, 2023    |
| Isotropic Field Probe | Rrankonia    | EP-601            | 611WX80275 | Aug 21, 2023    |
| Amplifier             | SKET         | HAP_801000M-250W  | 201811050  | Aug 21, 2023    |
| Amplifier             | SKET         | HAP_0103G-75W     | 201811051  | Aug 21, 2023    |
| Amplifier             | SKET         | HAP_0306G-20W     | 201811052  | Aug 21, 2023    |
| Log-periodic Antenna  | SKET         | ZDSZ-80T1000M-231 | SKT231015  | Aug 21, 2023    |
| Log-periodic Antenna  | SKET         | ZDSZ-1T6G-232     | SKT232079  | Aug 21, 2023    |

**3.3.7. For electrical fast transient/burst immunity test**

| Name of Equipment  | Manufacturer | Model               | Serial No.    | Calibration Due |
|--------------------|--------------|---------------------|---------------|-----------------|
| EFT Tester         | HTEC         | HV1P16T/HCOM PACT52 | 170901/190901 | Aug 21, 2023    |
| EFT Coupling Clamp | HTEC         | HEFT 51-C           | 1416011       | Aug 21, 2023    |

**3.3.8. For surge immunity test**

| Name of Equipment | Manufacturer | Model   | Serial No. | Calibration Due |
|-------------------|--------------|---------|------------|-----------------|
| Surge Tester      | HTEC         | HCWG 71 | 174302     | Aug 21, 2023    |
| Surge Tester      | HTEC         | TCOMB 4 | 142103     | Aug 21, 2023    |
| Surge Tester      | HTEC         | HTSG 70 | 175002     | Aug 21, 2023    |

**3.3.9. For injected currents susceptibility test**

| Name of Equipment               | Manufacturer | Model       | Serial No.    | Calibration Due |
|---------------------------------|--------------|-------------|---------------|-----------------|
| C/S Test System                 | SCHLODER     | CDG-6000-25 | 126A1279/2014 | Aug 21, 2023    |
| Coupling Decoupling Network     | SCHLODER     | CDN-M2+3    | A2210251/2013 | Aug 21, 2023    |
| Electromagnetic Injection Clamp | Luthi        | EM101       | 36041         | Aug 21, 2023    |
| Test S/W                        | SCHLODER     | CDG/1.0.0.0 |               |                 |

**3.3.10. For power frequency magnetic field immunity test**

| Name of Equipment     | Manufacturer | Model | Serial No. | Calibration Due |
|-----------------------|--------------|-------|------------|-----------------|
| Magnetic Field Tester | HTEC         | HPFMF | 142104     | Aug 21, 2023    |



Report No.: PTC23071004802E-EM01

**3.3.11. For voltage dips and short interruptions immunity test**

| Name of Equipment | Manufacturer | Model                  | Serial No.    | Calibration Due |
|-------------------|--------------|------------------------|---------------|-----------------|
| Dips Tester       | HTEC         | HV1P16T/HCOM<br>PACT52 | 170901/190901 | Aug 21, 2023    |



#### 4. EUT DESCRIPTION

|                         |                       |
|-------------------------|-----------------------|
| <b>Product</b>          | MULTI-FIELD EMF METER |
| <b>Model</b>            | HT627                 |
| <b>Supplied Voltage</b> | 1.5V*3 AAA Battery    |
| <b>Power</b>            | N/A                   |

#### I/O PORT

| I/O PORT TYPES | Q'TY | TESTED WITH                         |
|----------------|------|-------------------------------------|
| AC Port        | 1    | <input type="checkbox"/>            |
| DC Port        | 1    | <input checked="" type="checkbox"/> |

#### Models Difference

N/A

## 5. TEST METHODOLOGY

### 5.1. TEST MODE

The EUT was tested together with the thereafter additional components, and a configuration, which produced the worst emission levels, was selected and recorded in this report.

The following test mode(s) were assessed.

| Test Items |                                | Test Mode |
|------------|--------------------------------|-----------|
| Emission   | Conducted Emission             | N/A       |
|            | Radiated Emission              | Working   |
|            | Harmonic current emissions     | N/A       |
|            | Voltage fluctuations & flicker | N/A       |
| Immunity   | ESD                            | Working   |
|            | RS                             | Working   |
|            | EFT                            | N/A       |
|            | Surge                          | N/A       |
|            | C/S                            | N/A       |
|            | PFMF                           | N/A       |
|            | Dips                           | N/A       |

### 5.2. EUT SYSTEM OPERATION

1. Set up EUT with the support equipment.
2. Make sure the EUT work normally during the test.



## 6. SETUP OF EQUIPMENT UNDER TEST

### 6.1. DESCRIPTION OF SUPPORT UNITS


The EUT has been tested as an independent unit together with other necessary accessories or support units. The following support units or accessories were used to form a representative test configuration during the tests.

| No. | Equipment | Model | Serial No. | FCC ID | Trade Name | Data Cable | Power Cord |
|-----|-----------|-------|------------|--------|------------|------------|------------|
| 1.  | N/A       | N/A   | N/A        | N/A    | N/A        | N/A        | N/A        |

Note: 1) All the equipment/cables were placed in the worst-case configuration to maximize the emission during the test.

2) Grounding was established in accordance with the manufacturer's requirements and conditions for the intended use.

### 6.2. CONFIGURATION OF SYSTEM UNDER TEST



(EUT: MULTI-FIELD EMF METER)

## 7. EMISSION TEST

### 7.1. CONDUCTED EMISSION MEASUREMENT

#### 7.1.1. LIMITS

| FREQUENCY<br>(MHz) | Class A                    |                         | Class B                    |                         |
|--------------------|----------------------------|-------------------------|----------------------------|-------------------------|
|                    | Quasi-peak<br>dB( $\mu$ V) | Average<br>dB( $\mu$ V) | Quasi-peak<br>dB( $\mu$ V) | Average<br>dB( $\mu$ V) |
| 0.15 - 0.5         | 79                         | 66                      | 66-56                      | 56-46                   |
| 0.5 - 5.0          | 73                         | 60                      | 56                         | 46                      |
| 5.0 - 30.0         | 73                         | 60                      | 60                         | 50                      |

Note: 1) The lower limit shall apply at the transition frequencies.

2) The limit decreases in line with the logarithm of the frequency in the range of 0.15 to 0.50 MHz.

#### 7.1.2. TEST PROCEDURES


The EUT and Support equipment, if needed, was set up as per the test configuration to simulate typical usage per the user's manual. When the EUT is a tabletop system, a wooden table with a height of 0.8 meters is used and is placed on the ground plane. When the EUT is floor standing equipment, it is placed on the ground plane, which has a 3-12 mm non-conductive covering to insulate the EUT from the ground plane. The EUT should be 0.8 m apart from the AMN, where the mains cable supplied by the manufacturer is longer than 1 m, the excess should be folded at the centre into a bundle no longer than 0.4 m, Details please refer to test setup photography.

The Receiver scanned from 150 kHz to 30 MHz for emissions in each of the test modes. During the above scans, the emissions were maximized by cable manipulation.

A scan was taken on both of the power lines, Line and neutral, recording at least the six highest emissions. Emission frequency and amplitude were recorded into a computer in which correction factors were used to calculate the emission level and compare reading to the applicable limit. The test data of the worst-case condition(s) was recorded.

Note: Test Software Name: e3, Software Version: 1.0.0.0.

### 7.1.3. TEST SETUP

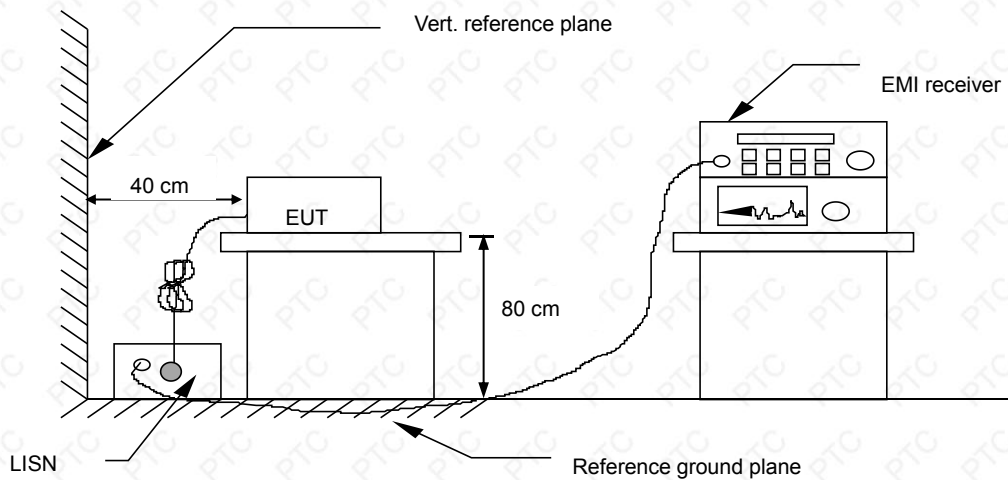

For the actual test configuration, please refer to the related item – Photographs of the Test Configuration.

### 7.1.4. TEST RESULT

N/A



## 7.2. RADIATED EMISSION MEASUREMENT

### 7.2.1. LIMITS

| FREQUENCY<br>(MHz) | Class A(At 3m)               | Class B(At 3m)               |
|--------------------|------------------------------|------------------------------|
|                    | Quasi-peak<br>dB( $\mu$ V/m) | Quasi-peak<br>dB( $\mu$ V/m) |
| 30 ~ 230           | 50                           | 40                           |
| 230 ~ 1000         | 57                           | 47                           |

Note: 1) The lower limit shall apply at the transition frequencies.

2) Emission level (dB $\mu$ V/m) = 20 log Emission level ( $\mu$ V/m).

### 7.2.2. TEST PROCEDURE

The equipment was set up as per the test configuration to simulate typical usage per the user's manual. When the EUT is a tabletop system, a wooden turntable with a height of 0.8 meters is used which is placed on the ground plane. When the EUT is floor standing equipment, it is placed on the ground plane which has a 0.1 m non-conductive covering to insulate the EUT from the ground plane.

The antenna was placed at 3 meter away from the EUT. The antenna connected to the spectrum analyzer via a cable and at times a pre-amplifier would be used.


The analyzer / receiver quickly scanned from 30 MHz to 1000 MHz. The EUT test program was started. Emissions were scanned and measured rotating the EUT to 360 degrees and positioning the antenna 1 to 4 meters above the ground plane, in both the vertical and the horizontal polarization, to maximize the emission reading level.

During the above scans, the emissions were maximized by cable manipulation. Each modes is measured, recorded at least the six highest emissions. The emission frequency, amplitude, antenna position, polarization and turntable position were recorded into a computer in which correction factors were used to calculate the emission level and compare reading to the applicable limit and only Q.P. reading is presented.

The test data of the worst-case condition(s) was recorded.

Note: Test Software Name: e3, Software Version: 8.2.1.0.

### 7.2.3. TEST SETUP

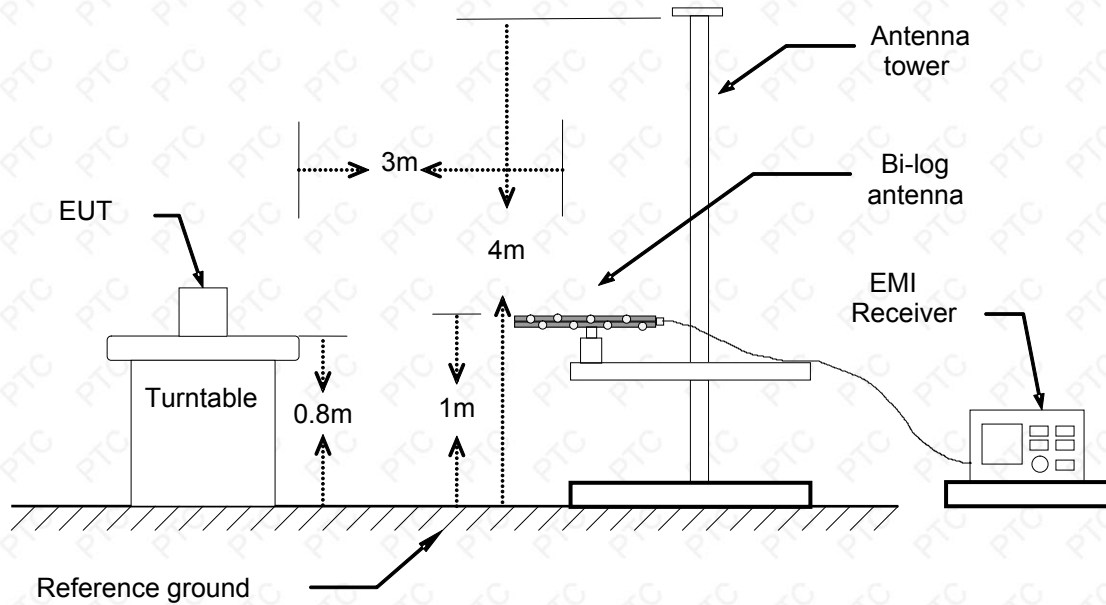

For the actual test configuration, please refer to the related item – Photographs of the Test Configuration

### 7.2.4. TEST RESULT

|                                 |                          |                          |                       |
|---------------------------------|--------------------------|--------------------------|-----------------------|
| <b>Product name</b>             | MULTI-FIELD EMF METER    | <b>Antenna Distance</b>  | 3 m                   |
| <b>Model</b>                    | HT627                    | <b>Antenna Pole</b>      | Vertical / Horizontal |
| <b>Test Mode</b>                | Working                  | <b>Detector Function</b> | Peak / Quasi-peak     |
| <b>Environmental Conditions</b> | 25°C, 60 % RH, 101.5 kPa | <b>6 dB Bandwidth</b>    | 120 kHz               |
| <b>Tested by</b>                | Mickey                   | <b>Test Result</b>       | Pass                  |

Note:

Freq. = Emission frequency in MHz

Reading level (dBμV) = Receiver reading(dBμV)

Corr.Factor (dB/m)=Antenna factor(dB/m)+Cable loss(dB)-Preamp Factor(dB)

Measurement (dBμV/m)=Reading level(dBμV)+ Corr. Factor (dB/m)

Limit (dBμV/m) = Limit stated in standard

Over Limit (dB) = Measurement (dBμV/m) – Limit (dBμV/m)

QP = Quasi-Peak

The highest frequency of the internal sources of the EUT was less than 108 MHz, so the measurement was only made up to 1 GHz.



Please refer to the following diagram:

Vertical:




Final Data List[QP]

| NO. | Freq. [MHz] | QP Reading [dBμV] | Factor [dB/m] | QP Value [dBμV/m] | QP Limit [dBμV/m] | QP Margin [dB] | Polarity | Verdict |
|-----|-------------|-------------------|---------------|-------------------|-------------------|----------------|----------|---------|
| 1   | 32.91       | 33.07             | -15.18        | 17.89             | 40.00             | 22.11          | Vertical | PASS    |
| 2   | 148.34      | 38.96             | -18.77        | 20.19             | 40.00             | 19.81          | Vertical | PASS    |
| 3   | 168.71      | 37.68             | -19.33        | 18.35             | 40.00             | 21.65          | Vertical | PASS    |
| 4   | 637.22      | 34.80             | -9.34         | 25.46             | 47.00             | 21.54          | Vertical | PASS    |
| 5   | 833.16      | 33.23             | -6.77         | 26.46             | 47.00             | 20.54          | Vertical | PASS    |
| 6   | 988.36      | 33.12             | -5.15         | 27.97             | 47.00             | 19.03          | Vertical | PASS    |



Horizontal:

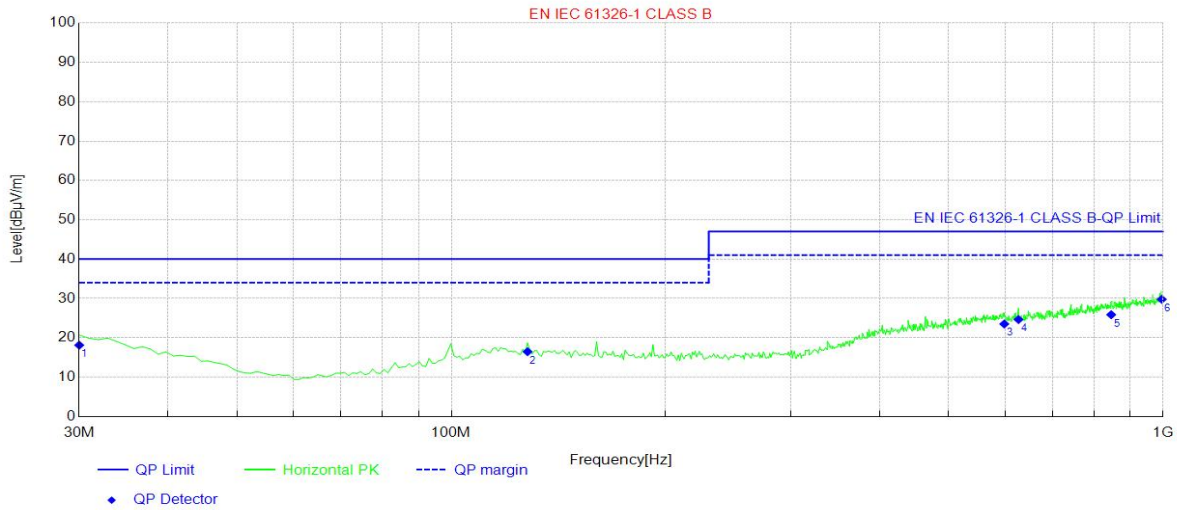

| Final Data List[QP] |                |                         |                  |                      |                      |                   |            |         |
|---------------------|----------------|-------------------------|------------------|----------------------|----------------------|-------------------|------------|---------|
| NO.                 | Freq.<br>[MHz] | QP<br>Reading<br>[dBμV] | Factor<br>[dB/m] | QP Value<br>[dBμV/m] | QP Limit<br>[dBμV/m] | QP Margin<br>[dB] | Polarity   | Verdict |
| 1                   | 30.00          | 31.89                   | -13.76           | 18.13                | 40.00                | 21.87             | Horizontal | PASS    |
| 2                   | 127.97         | 34.24                   | -17.77           | 16.47                | 40.00                | 23.53             | Horizontal | PASS    |
| 3                   | 598.42         | 32.75                   | -9.24            | 23.51                | 47.00                | 23.49             | Horizontal | PASS    |
| 4                   | 626.55         | 33.94                   | -9.29            | 24.65                | 47.00                | 22.35             | Horizontal | PASS    |
| 5                   | 845.77         | 32.34                   | -6.47            | 25.87                | 47.00                | 21.13             | Horizontal | PASS    |
| 6                   | 996.12         | 35.02                   | -5.24            | 29.78                | 47.00                | 17.22             | Horizontal | PASS    |

## 7.3. HARMONICS CURRENT MEASUREMENT

### 7.3.1. LIMITS OF HARMONICS CURRENT MEASUREMENT

| Limit for Class A equipment |                                      |
|-----------------------------|--------------------------------------|
| Harmonics Order N           | Max. permissible harmonics current A |
| Odd harmonics               |                                      |
| 3                           | 2.30                                 |
| 5                           | 1.14                                 |
| 7                           | 0.77                                 |
| 9                           | 0.40                                 |
| 11                          | 0.33                                 |
| 13                          | 0.21                                 |
| $15 \leq n \leq 39$         | $0.15 \times (15/n)$                 |
| Even harmonics              |                                      |
| 2                           | 1.08                                 |
| 4                           | 0.43                                 |
| 6                           | 0.30                                 |
| $8 \leq n \leq 40$          | $0.23 \times 8/n$                    |

| Limit for Class D equipment                 |                                                  |                                      |
|---------------------------------------------|--------------------------------------------------|--------------------------------------|
| Harmonics Order n                           | Max. permissible harmonics current per watt mA/W | Max. permissible harmonics current A |
| Odd Harmonics only                          |                                                  |                                      |
| 3                                           | 3.4                                              | 2.30                                 |
| 5                                           | 1.9                                              | 1.14                                 |
| 7                                           | 1.0                                              | 0.77                                 |
| 9                                           | 0.5                                              | 0.40                                 |
| 11                                          | 0.35                                             | 0.33                                 |
| 13                                          | 0.30                                             | 0.21                                 |
| $15 \leq n \leq 39$<br>(odd harmonics only) | $3.85/n$                                         | $0.15 \times (15/n)$                 |
|                                             |                                                  |                                      |
|                                             |                                                  |                                      |
|                                             |                                                  |                                      |
|                                             |                                                  |                                      |

| Limit for Class C equipment <sup>a</sup>      |                                                                                                                  |
|-----------------------------------------------|------------------------------------------------------------------------------------------------------------------|
| Harmonics Order n                             | Max. permissible harmonics current expressed as a percentage of the input current at the fundamental frequency A |
| 2                                             | 2                                                                                                                |
| 3                                             | 27 <sup>b</sup>                                                                                                  |
| 5                                             | 10                                                                                                               |
| 7                                             | 7                                                                                                                |
| 9                                             | 5                                                                                                                |
| $11 \leq n < \leq 39$<br>(odd harmonics only) | 3                                                                                                                |

<sup>a</sup>:For some Class C products, other emission limits apply (see BS EN IEC 61000-3-2 7.4).

<sup>b</sup>:The limit is determined based on the assumption of modern lighting technologies having power factors of 0,90 or higher

Note: Class A, B, C and D are classified according to item 7.3.2.of this report

### 7.3.2. TEST PROCEDURES

The EUT was placed on the top of a wooden table 0.8 meters above the ground and operated to produce the maximum harmonic. The classification of EUT is according to section 5 of EN IEC 61000-3-2.

The EUT is classified as follows:

Class A:

Equipment not specified as belonging to Class B, C or D shall be considered as Class A equipment.

Some examples of Class A equipment are:

- balanced three-phase equipment;
- household appliances, excluding those specified as belonging to Class B, C or D;
- vacuum cleaners;
- high pressure cleaners;
- tools, excluding portable tools;
- independent phase control dimmers;
- audio equipment;
- professional luminaires for stage lighting and studios.

NOTE 1 Equipment that can be shown to have a significant effect on the supply system might be reclassified in a future edition of this document, taking into account the following factors:

- number of pieces of equipment in use;
- duration of use;
- simultaneity of use;
- power consumption;
- harmonic spectrum, including phase.

Class B:

- portable tools;
- arc welding equipment which is not professional equipment.

Class C:

- lighting equipment.

Class D:

Equipment having a specified power less than or equal to 600 W according to 6.3.2, of the following types:


- personal computers and personal computer monitors;

- television receivers;
- refrigerators and freezers having one or more variable-speed drives to control compressor motor(s).

NOTE 2 Class D limits are reserved for equipment that, by virtue of the factors listed in note 1 , can be shown to have a pronounced effect on the public electricity supply system.

The correspondent test program of test instrument to measure the current harmonics emanated from EUT is chosen. The measure time shall be not less than the time necessary for the EUT to be exercised.

### 7.3.3. TEST SETUP

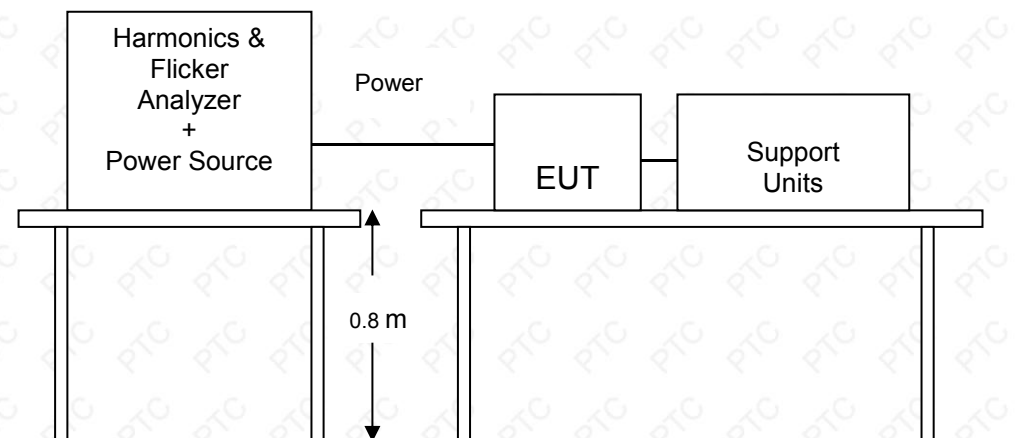

For the actual test configuration, please refer to the related item – Photographs of the Test Configuration.

### 7.3.4. TEST RESULT

N/A

## 7.4. VOLTAGE FLUCTUATION AND FLICKS MEASUREMENT


### 7.4.1. LIMITS OF VOLTAGE FLUCTUATION AND FLICKS MEASUREMENT

| TEST ITEM     | LIMIT   | REMARK                                             |
|---------------|---------|----------------------------------------------------|
| $P_{st}$      | 1.0     | $P_{st}$ means short-term flicker indicator.       |
| $P_{lt}$      | 0.65    | $P_{lt}$ means long-term flicker indicator.        |
| $T_{dt}$ (ms) | 500     | $T_{dt}$ means maximum time that $dt$ exceeds 3 %. |
| $d_{max}$ (%) | 4/6/7 % | $d_{max}$ means maximum relative voltage change.   |
| $dc$ (%)      | 3.3 %   | $dc$ means relative steady-state voltage change    |

### 7.4.2. TEST PROCEDURE

The EUT was placed on the top of a wooden table 0.8 meters above the ground and operated to produce the most unfavorable sequence of voltage changes under Working operating conditions. During the flick measurement, the measure time shall include that part of whole operation cycle in which the EUT produce the most unfavorable sequence of voltage changes. The observation period for short-term flicker indicator is 10 minutes and the observation period for long-term flicker indicator is 2 hours.

### 7.4.3. TEST SETUP

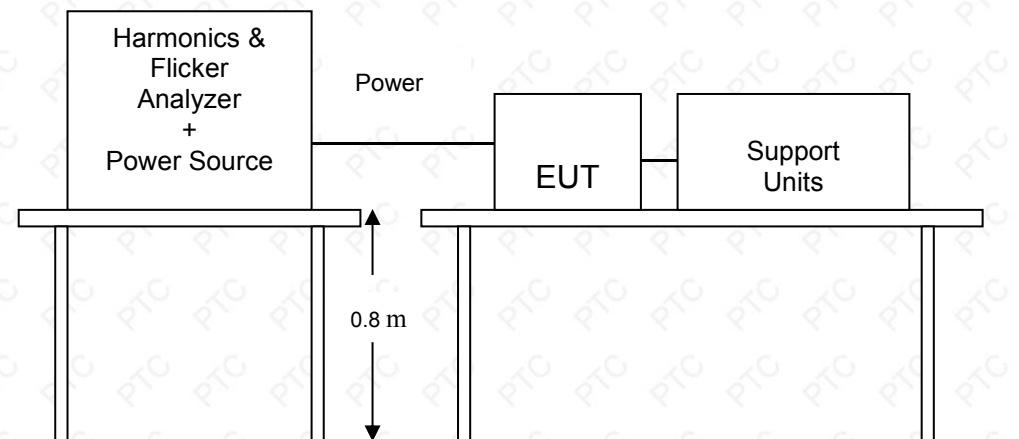

For the actual test configuration, please refer to the related item – Photographs of the Test Configuration.

### 7.4.4. TEST RESULT

N/A

## 8. IMMUNITY TEST

### 8.1. GENERAL DESCRIPTION

**Table1 – Immunity test requirements for equipment intended to be used in a BASIC ELECTROMAGNETIC ENVIRONMENT**

| PORT                                                                  | Phenomenon                                  | Basic standard | Test value                                                                           | Performance criterion |
|-----------------------------------------------------------------------|---------------------------------------------|----------------|--------------------------------------------------------------------------------------|-----------------------|
| ENCLOSURE                                                             | ESD                                         | IEC 61000-4-2  | ±4 kV contact discharge<br>±8 kV air discharge                                       | B<br>B                |
|                                                                       | Electromagnetic field                       | IEC 61000-4-3  | 3 V/m (80 MHz to 1 GHz;<br>1,4 GHz to 6 GHz) <sup>a</sup>                            | A                     |
|                                                                       | Power frequency magnetic field <sup>b</sup> | IEC 61000-4-8  | 3 A/m (50 Hz, 60 Hz)                                                                 | A                     |
| AC power<br>(including protective earth)                              | Burst                                       | IEC 61000-4-4  | ±1 kV (5 kHz or 100 kHz)                                                             | B                     |
|                                                                       | Surge                                       | IEC 61000-4-5  | ±0,5 kV line-to-line<br>±1 kV line-to-ground                                         | B<br>B                |
|                                                                       | Conducted RF                                | IEC 61000-4-6  | 3 V (150 kHz to 80 MHz)                                                              | A                     |
|                                                                       | Voltage dip                                 | IEC 61000-4-11 | 0 % during half cycle<br>0 % during 1 cycle<br>70 % during 25/30 cycles <sup>c</sup> | B<br>B<br>C           |
|                                                                       | Short interruptions                         | IEC 61000-4-11 | 0 % during 250/300 cycles <sup>c</sup>                                               | C                     |
| DC power <sup>d, e</sup><br>(including protective earth)              | Burst                                       | IEC 61000-4-4  | ±1 kV (5 kHz or 100 kHz)                                                             | B                     |
|                                                                       | Surge                                       | IEC 61000-4-5  | ±0,5 kV line-to-line<br>±1 kV line-to-ground                                         | B<br>B                |
|                                                                       | Conducted RF                                | IEC 61000-4-6  | 3 V (150 kHz to 80 MHz)                                                              | A                     |
| I/O signal/control <sup>e</sup><br>(including functional earth)       | Burst <sup>d</sup>                          | IEC 61000-4-4  | ±0,5 kV (5 kHz or 100 kHz)                                                           | B                     |
|                                                                       | Surge <sup>f</sup>                          | IEC 61000-4-5  | ±1 kV line-to-ground                                                                 | B                     |
|                                                                       | Conducted RF <sup>d</sup>                   | IEC 61000-4-6  | 3 V (150 kHz to 80 MHz)                                                              | A                     |
| I/O signal/control <sup>e</sup><br>connected directly to mains supply | Burst <sup>d</sup>                          | IEC 61000-4-4  | ±1 kV (5 kHz or 100 kHz)                                                             | B                     |
|                                                                       | Surge <sup>f</sup>                          | IEC 61000-4-5  | ±0,5 kV line-to-line<br>±1 kV line-to-ground                                         | B<br>B                |
|                                                                       | Conducted RF <sup>d</sup>                   | IEC 61000-4-6  | 3 V (150 kHz to 80 MHz)                                                              | A                     |

<sup>a</sup> In case testing is performed also in the frequency range from 1 GHz to 1,4 GHz, the same test level is recommended.

<sup>b</sup> Only to magnetically sensitive equipment.

<sup>c</sup> For example, "25/30 cycles" means "25 cycles for 50 Hz test" or "30 cycles for 60 Hz test".

<sup>d</sup> Only in the case of lines >3 m.

<sup>e</sup> DC POWER PORTS intended to be connected to a low voltage DC supply (≤ 60 V), where secondary circuits (isolated from the AC mains supply) are not subject to transient overvoltages (i.e. reliably-grounded, capacitively-filtered DC secondary circuits) shall be regarded as I/O signal/control PORTS.

<sup>f</sup> Only in the case of LONG-DISTANCE LINES.

**Table 2 – Immunity test requirements for equipment intended to be used in an INDUSTRIAL ELECTROMAGNETIC ENVIRONMENT**

| PORT                                                                    | Phenomenon                                  | Basic standard | Test value                                                                                           | Performance criterion |
|-------------------------------------------------------------------------|---------------------------------------------|----------------|------------------------------------------------------------------------------------------------------|-----------------------|
| ENCLOSURE                                                               | ESD                                         | IEC 61000-4-2  | ±4 kV contact discharge<br>±8 kV air discharge                                                       | B<br>B                |
|                                                                         | Electromagnetic field                       | IEC 61000-4-3  | 10 V/m (80 MHz to 1 GHz)<br>3 V/m (1,4 GHz to 6 GHz) <sup>a</sup>                                    | A<br>A                |
|                                                                         | Power frequency magnetic field <sup>b</sup> | IEC 61000-4-8  | 30 A/m (50 Hz, 60 Hz)                                                                                | A                     |
| AC power<br>(including protective earth)                                | Burst                                       | IEC 61000-4-4  | ±2 kV (5 kHz or 100 kHz)                                                                             | B                     |
|                                                                         | Surge                                       | IEC 61000-4-5  | ±1 kV line-to-line<br>±2 kV line-to-ground                                                           | B<br>B                |
|                                                                         | Conducted RF                                | IEC 61000-4-6  | 3 V (150 kHz to 80 MHz),<br>see NOTE                                                                 | A                     |
|                                                                         | Voltage dip                                 | IEC 61000-4-11 | 0 % during 1 cycle<br>40 % during 10/12 cycles <sup>c</sup><br>70 % during 25/30 cycles <sup>c</sup> | B<br>C<br>C           |
|                                                                         | Short interruptions                         | IEC 61000-4-11 | 0 % during 250/300 cycles <sup>c</sup>                                                               | C                     |
| DC power <sup>d, e</sup><br>(including protective earth)                | Burst                                       | IEC 61000-4-4  | ±2 kV (5 kHz or 100 kHz)                                                                             | B                     |
|                                                                         | Surge                                       | IEC 61000-4-5  | ±1 kV line-to-line<br>±2 kV line-to-ground                                                           | B<br>B                |
|                                                                         | Conducted RF                                | IEC 61000-4-6  | 3 V (150 kHz to 80 MHz)<br>see NOTE                                                                  | A                     |
| I/O signal/control <sup>e</sup><br>(including functional earth)         | Burst <sup>d</sup>                          | IEC 61000-4-4  | ±1 kV (5 kHz or 100 kHz)                                                                             | B                     |
|                                                                         | Surge <sup>f</sup>                          | IEC 61000-4-5  | ±1 kV line-to-ground                                                                                 | B                     |
|                                                                         | Conducted RF <sup>d</sup>                   | IEC 61000-4-6  | 3 V (150 kHz to 80 MHz)<br>see NOTE                                                                  | A                     |
| I/O signal/control <sup>e</sup><br>(connected directly to mains supply) | Burst <sup>d</sup>                          | IEC 61000-4-4  | ±2 kV (5 kHz or 100 kHz)                                                                             | B                     |
|                                                                         | Surge <sup>f</sup>                          | IEC 61000-4-5  | ±1 kV line-to-line<br>±2 kV line-to-ground                                                           | B<br>B                |
|                                                                         | Conducted RF <sup>d</sup>                   | IEC 61000-4-6  | 3 V (150 kHz to 80 MHz)<br>see NOTE                                                                  | A                     |

NOTE Equipment considered in this table is typically used in industrial installations with the cabling arranged on metallic structures. This reduces coupling of electromagnetic fields into cables and hence justifies a lower immunity level compared to that given in the generic immunity standard IEC 61000-6-2. The level of 3 V is used for more than 15 years without immunity issues and hence proved to be sufficient.

<sup>a</sup> In case testing is performed also in the frequency range from 1 GHz to 1,4 GHz, the same test level as above 1,4 GHz is recommended.

<sup>b</sup> Only to magnetically sensitive equipment.

<sup>c</sup> For example, "25/30 cycles" means "25 cycles for 50 Hz test" or "30 cycles for 60 Hz test".

<sup>d</sup> Only in the case of lines > 3 m.

<sup>e</sup> DC power PORTS intended to be connected to a low voltage DC supply (≤ 60 V), where secondary circuits (isolated from the AC mains supply) are not subject to transient overvoltages (i.e. reliably-grounded, capacitively-filtered DC secondary circuits) shall be regarded as I/O signal/control PORTS.

<sup>f</sup> Only in the case of LONG-DISTANCE LINES.

**Table 3 – Immunity test requirements for equipment intended to be used in a CONTROLLED ELECTROMAGNETIC ENVIRONMENT**

| PORT                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                       | Phenomenon                | Basic standard | Test value                                                | Performance criterion |
|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|---------------------------|----------------|-----------------------------------------------------------|-----------------------|
| ENCLOSURE                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                  | ESD                       | IEC 61000-4-2  | ±4 kV contact discharge<br>±8 kV air discharge            | B<br>B                |
|                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                            | Electromagnetic field     | IEC 61000-4-3  | 1 V/m (80 MHz to 1 GHz;<br>1,4 GHz to 6 GHz) <sup>a</sup> | A                     |
| AC power<br>(including protective earth)                                                                                                                                                                                                                                                                                                                                                                                                                                                                   | Burst                     | IEC 61000-4-4  | ±1 kV (5 kHz or 100 kHz)                                  | B                     |
|                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                            | Surge                     | IEC 61000-4-5  | ±0,5 kV line-to-line<br>±1 kV line-to-ground              | B<br>B                |
|                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                            | Conducted RF              | IEC 61000-4-6  | 1 V (150 kHz to 80 MHz)                                   | A                     |
| DC power <sup>b, c</sup><br>(including protective earth)                                                                                                                                                                                                                                                                                                                                                                                                                                                   | Burst                     | IEC 61000-4-4  | ±1 kV (5 kHz or 100 kHz)                                  | B                     |
|                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                            | Conducted RF              | IEC 61000-4-6  | 1 V (150 kHz to 80 MHz)                                   | A                     |
| I/O signal/control <sup>c</sup><br>(including functional earth)                                                                                                                                                                                                                                                                                                                                                                                                                                            | Burst <sup>b</sup>        | IEC 61000-4-4  | ±0,5 kV (5 kHz or 100 kHz)                                | B                     |
|                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                            | Conducted RF <sup>b</sup> | IEC 61000-4-6  | 1 V (150 kHz to 80 MHz)                                   | A                     |
| <sup>a</sup> In case testing is performed also in the frequency range from 1 GHz to 1,4 GHz, the same test level is recommended.<br><sup>b</sup> Only in the case of lines > 3 m.<br><sup>c</sup> DC power PORTS intended to be connected to a low voltage DC supply (≤ 60 V), where secondary circuits (isolated from the AC mains supply) are not subject to transient overvoltages (i.e. reliably-grounded, capacitively-filtered DC secondary circuits) shall be regarded as I/O signal/control PORTS. |                           |                |                                                           |                       |



## 8.2. GENERAL PERFORMANCE CRITERIA DESCRIPTION

|                    |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                         |
|--------------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Criteria A:</b> | During and after the test the EUT shall continue to operate as intended without operator intervention. No degradation of performance or loss of function is allowed below a minimum performance level specified by the manufacturer when the EUT is used as intended. The performance level may be replaced by a permissible loss of performance. If the minimum performance level or the permissible performance loss is not specified by the manufacturer, then either of these may be derived from the product description and documentation, and by what the user may reasonably expect from the EUT if used as intended.                                                                                                                                                                                           |
| <b>Criteria B:</b> | <p>After the test, the EUT shall continue to operate as intended without operator intervention. No degradation of performance or loss of function is allowed, after the application of the phenomena below a performance level specified by the manufacturer, when the EUT is used as intended. The performance level may be replaced by a permissible loss of performance.</p> <p>During the test, degradation of performance is allowed. However, no change of operating state or stored data is allowed to persist after the test. If the minimum performance level (or the permissible performance loss) is not specified by the manufacturer, then either of these may be derived from the product description and documentation, and by what the user may reasonably expect from the EUT if used as intended.</p> |
| <b>Criteria C:</b> | <p>During and after testing, a temporary loss of function is allowed, provided the function is self-recoverable, or can be restored by the operation of the controls or cycling of the power to the EUT by the user in accordance with the manufacturer's instructions.</p> <p>Functions, and/or information stored in non-volatile memory, or protected by a battery backup, shall not be lost.</p>                                                                                                                                                                                                                                                                                                                                                                                                                    |

### 8.3. ELECTROSTATIC DISCHARGE (ESD)

#### 8.3.1. TEST SPECIFICATION

|                               |                                                                                       |
|-------------------------------|---------------------------------------------------------------------------------------|
| <b>Basic Standard:</b>        | IEC 61000-4-2                                                                         |
| <b>Discharge Impedance:</b>   | 330 $\Omega$                                                                          |
| <b>Charging Capacity:</b>     | 150 pF                                                                                |
| <b>Discharge Voltage:</b>     | Air Discharge: $\pm 8$ kV (Direct)<br>Contact Discharge: $\pm 4$ kV (Direct/Indirect) |
| <b>Polarity:</b>              | Positive & Negative                                                                   |
| <b>Number of Discharge:</b>   | 10                                                                                    |
| <b>Discharge Mode:</b>        | 1 time/s                                                                              |
| <b>Performance Criterion:</b> | B                                                                                     |

#### 8.3.2. TEST PROCEDURE

The discharges shall be applied in two ways:


- Contact discharges to the conductive surfaces and coupling planes:  
50 dischargers (10 times positive and 10 times negative polarity) shall be applied on each accessible metallic part of the enclosure, terminals are excluded. In case of a non-conductive enclosure, dischargers shall be applied on the horizontal or vertical coupling planes. Test shall be performed at a maximum repetition rate of one discharge per second.
- Air discharges at slots and apertures and insulating surfaces:  
On those parts of the EUT where it is not possible to perform contact discharge testing, the equipment should be investigated to identify user accessible points where breakdown may occur. Such points are tested using the air discharge method. This investigation should be restricted to those area normally handled by the user. A minimum of 10 single air discharges shall be applied to the selected test point for each such area.

The basic test procedure was in accordance with IEC 61000-4-2:

- The EUT was located 0.1 m minimum from all side of the HCP (dimensions 1.6 m x 0.8 m).
- The support units were located another table 30 cm away from the EUT, but direct support unit was/were located at same location as EUT on the HCP and keep at a distance of 10cm with EUT.
- The time interval between two successive single discharges was at least 1 second.

- d) Contact discharges were applied to the non-insulating coating, with the pointed tip of the generator penetrating the coating and contacting the conducting substrate.
- e) Air discharges were applied with the round discharge tip of the discharge electrode approaching the EUT as fast as possible (without causing mechanical damage) to touch the EUT. After each discharge, the ESD generator was removed from the EUT and re-triggered for a new single discharge. The test was repeated until all discharges were complete.
- f) At least ten single discharges (in the most sensitive polarity) were applied at the front edge of each HCP opposite the center point of each unit of the EUT and 0.1 meter from the front of the EUT. The long axis of the discharge electrode was in the plane of the HCP and perpendicular to its front edge during the discharge.
- g) At least ten single discharges (in the most sensitive polarity) were applied to the center of one vertical edge of the Vertical Coupling Plane (VCP) in sufficiently different positions that the four faces of the EUT were completely illuminated. The VCP (dimensions 0.5 m x 0.5 m) was placed vertically to and 0.1 meter from the EUT.

### 8.3.3. TEST SETUP

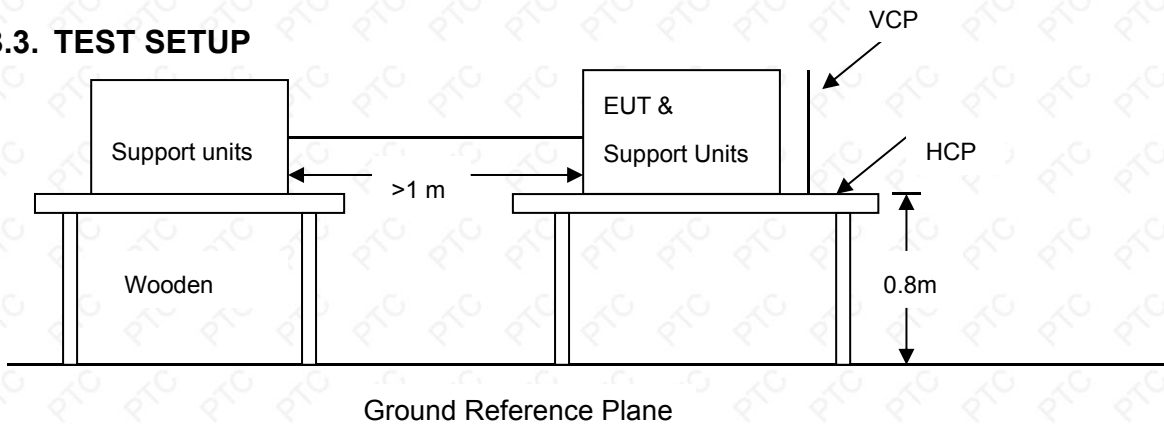

For the actual test configuration, please refer to the related item – Photographs of the Test Configuration.

Note:

#### 1) TABLE-TOP EQUIPMENT

The configuration consisted of a wooden table 0.8 meters high standing on the ground reference plane (GRP). The GRP consisted of a sheet of aluminum at least 0.25 mm thick, and 2.5 meters square connected to the protective grounding system. A horizontal coupling plane (HCP) (1.6 m x 0.8 m) was placed on the table and attached to the GRP by means of a cable with 940k total impedance. The equipment under test, was installed in a representative system as described in section 7 of IEC 61000-4-2, and its cables were placed on the HCP and isolated by an insulating support of 0.5 mm thickness. A distance of 1-meter minimum was provided between the EUT and the walls of the laboratory and any other metallic structure.

#### 2) FLOOR-STANDING EQUIPMENT

The equipment under test was installed in a representative system as described in section 7 of IEC 61000-4-2, and its cables were isolated from the ground reference plane by an insulating support of 0.1 meter thickness. The GRP consisted of a sheet of aluminum that is at least 0.25 mm thick, and 2.5 meters square connected to the protective grounding system and extended at least 0.5 meters from the EUT on all sides.



### 8.3.4. TEST RESULT

|                  |                       |                                 |                            |
|------------------|-----------------------|---------------------------------|----------------------------|
| <b>Product</b>   | MULTI-FIELD EMF METER | <b>Environmental Conditions</b> | 24.3°C, 52 % RH, 101.2 kPa |
| <b>Model</b>     | HT627                 | <b>Tested By</b>                | Bruce                      |
| <b>Test mode</b> | Working               | <b>Test Result</b>              | Pass                       |

| Air Discharge |                                     |                                     |                          |                                                                                                  |                       |
|---------------|-------------------------------------|-------------------------------------|--------------------------|--------------------------------------------------------------------------------------------------|-----------------------|
| Test Points   | Test Levels                         | Results                             |                          |                                                                                                  |                       |
|               | ± 8 kV                              | Pass                                | Fail                     | Observation                                                                                      | Performance Criterion |
| Gap 6points   | <input checked="" type="checkbox"/> | <input checked="" type="checkbox"/> | <input type="checkbox"/> | Note <input checked="" type="checkbox"/> A <input type="checkbox"/> B <input type="checkbox"/> C | B                     |

| Contact Discharge |                                     |                                     |                          |                                                                                                  |                       |
|-------------------|-------------------------------------|-------------------------------------|--------------------------|--------------------------------------------------------------------------------------------------|-----------------------|
| Test Points       | Test Levels                         | Results                             |                          |                                                                                                  |                       |
|                   | ± 4 kV                              | Pass                                | Fail                     | Observation                                                                                      | Performance Criterion |
| HCP 4points       | <input checked="" type="checkbox"/> | <input checked="" type="checkbox"/> | <input type="checkbox"/> | Note <input checked="" type="checkbox"/> A <input type="checkbox"/> B <input type="checkbox"/> C | B                     |
| VCP 4points       | <input checked="" type="checkbox"/> | <input checked="" type="checkbox"/> | <input type="checkbox"/> | Note <input checked="" type="checkbox"/> A <input type="checkbox"/> B <input type="checkbox"/> C | B                     |

Note: A) There was no change compared with initial operation during the test.

B) During the test, degradation of performance is allowed. However, no change of operating state or stored data is allowed to persist after the test. If the minimum performance level (or the permissible performance loss) is not specified by the manufacturer, then either of these may be derived from the product description and documentation, and by what the user may reasonably expect from the EUT if used as intended.

C) During and after testing, a temporary loss of function is allowed, provided the function is self-recoverable, or can be restored by the operation of the controls or cycling of the power to the EUT by the user in accordance with the manufacturer's instructions.

## 8.4. RADIATED, RADIO-FREQUENCY, ELECTROMAGNETIC FIELD (RS)

### 8.4.1. TEST SPECIFICATION


|                               |                                      |
|-------------------------------|--------------------------------------|
| <b>Basic Standard:</b>        | IEC 61000-4-3                        |
| <b>Frequency Range:</b>       | 80MHz to 6GHz                        |
| <b>Field Strength:</b>        | 3V/m                                 |
| <b>Modulation:</b>            | 1 kHz Sine Wave, 80 %, AM Modulation |
| <b>Frequency Step:</b>        | 1 % of preceding frequency value     |
| <b>Polarity of Antenna:</b>   | Horizontal and Vertical              |
| <b>Test Distance:</b>         | 3 m                                  |
| <b>Antenna Height:</b>        | 1.5 m                                |
| <b>Performance Criterion:</b> | A                                    |

### 8.4.2. TEST PROCEDURE

The test procedure was in accordance with IEC 61000-4-3

- The testing was performed in a fully anechoic chamber. The transmit antenna was located at a distance of 3 meters from the EUT.
- The frequency range is swept from 80MHz to 1GHz, 1.4GHz to 2GHz, 2.0GHz to 2.7GHz, with the signal 80% amplitude modulated with a 1 kHz sine-wave. The rate of sweep did not exceed  $1.5 \times 10^{-3}$  decade/s, where the frequency range is swept incrementally, the step size was 1 % of preceding frequency value.
- The dwell time at each frequency shall be not less than the time necessary for the EUT to be able to respond.
- The test was performed with the EUT exposed to both vertically and horizontally polarized fields on each of the four sides.

### 8.4.3. TEST SETUP

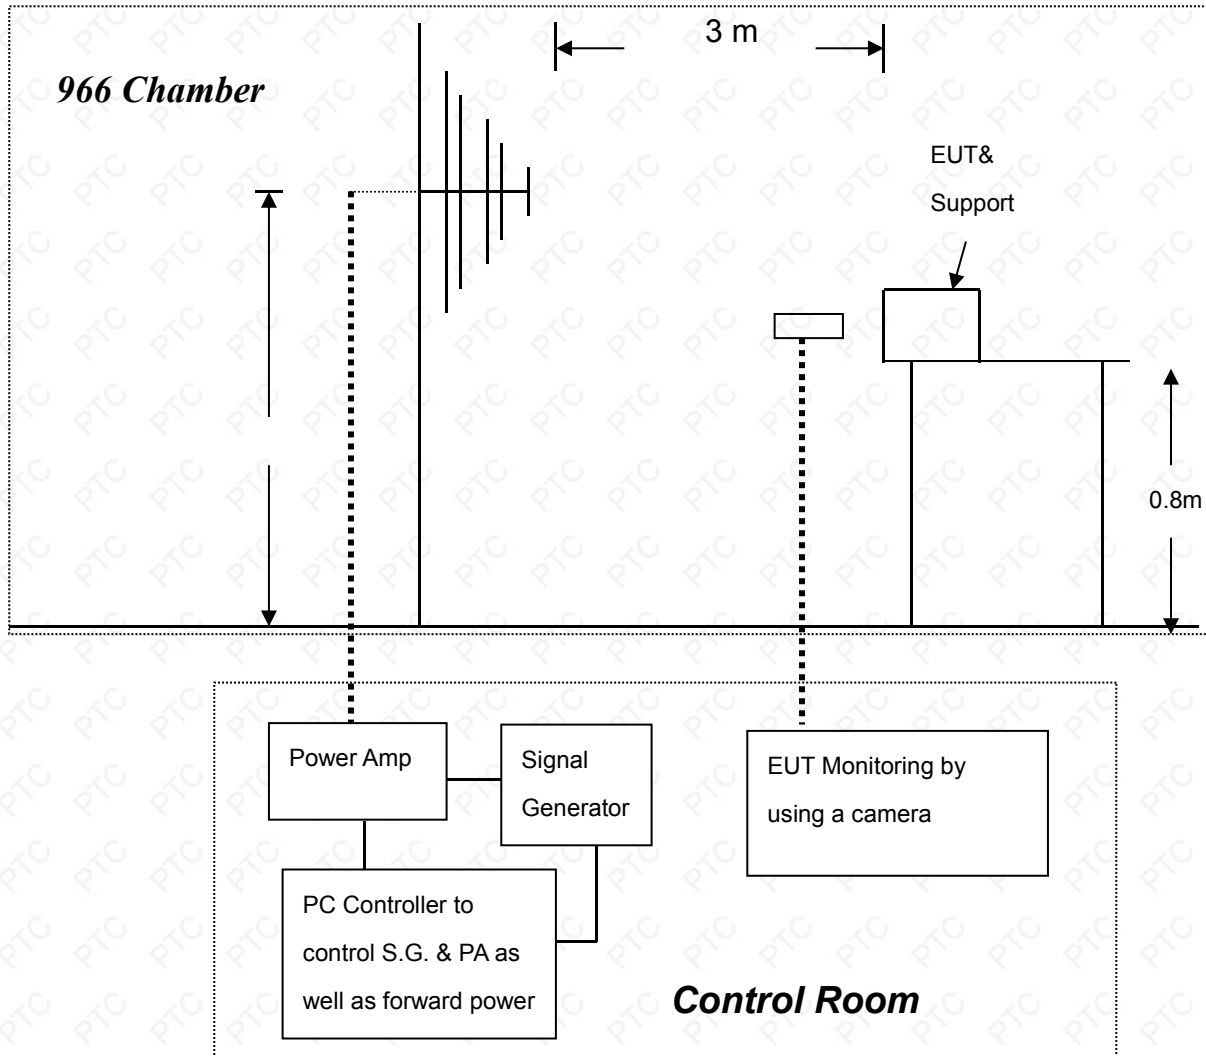

For the actual test configuration, please refer to the related item – Photographs of the Test Configuration.

Note:

#### TABLETOP EQUIPMENT

The EUT installed in a representative system as described in section 7 of IEC 61000-4-3 was placed on a non-conductive table 0.8 meters in height. The system under test was connected to the power and signal wire according to relevant installation instructions.

#### FLOOR STANDING EQUIPMENT

The EUT installed in a representative system as described in section 7 of IEC 61000-4-3 was placed on a non-conductive wood support 0.1 meters in height. The system under test was connected to the power and signal wire according to relevant installation instructions.



#### 8.4.4. TEST RESULT

|                  |                       |                                 |                            |
|------------------|-----------------------|---------------------------------|----------------------------|
| <b>Product</b>   | MULTI-FIELD EMF METER | <b>Environmental Conditions</b> | 24.1°C, 53 % RH, 101.1 kPa |
| <b>Model</b>     | HT627                 | <b>Tested By</b>                | Bruce                      |
| <b>Test mode</b> | Working               | <b>Test Result</b>              | Pass                       |

| Frequency (MHz)      | Polarity | Position | Field Strength (V/m) | Observation                                                                                      | Performance Criterion |
|----------------------|----------|----------|----------------------|--------------------------------------------------------------------------------------------------|-----------------------|
| 80-1000<br>1400-6000 | V&H      | Front    | 3                    | Note <input checked="" type="checkbox"/> A <input type="checkbox"/> B <input type="checkbox"/> C | A                     |
| 80-1000<br>1400-6000 | V&H      | Rear     | 3                    | Note <input checked="" type="checkbox"/> A <input type="checkbox"/> B <input type="checkbox"/> C | A                     |
| 80-1000<br>1400-6000 | V&H      | Left     | 3                    | Note <input checked="" type="checkbox"/> A <input type="checkbox"/> B <input type="checkbox"/> C | A                     |
| 80-1000<br>1400-6000 | V&H      | Right    | 3                    | Note <input checked="" type="checkbox"/> A <input type="checkbox"/> B <input type="checkbox"/> C | A                     |

Note: A) There was no change compared with initial operation during the test.

B) During the test, degradation of performance is allowed. However, no change of operating state or stored data is allowed to persist after the test. If the minimum performance level (or the permissible performance loss) is not specified by the manufacturer, then either of these may be derived from the product description and documentation, and by what the user may reasonably expect from the EUT if used as intended.

C) During and after testing, a temporary loss of function is allowed, provided the function is self-recoverable, or can be restored by the operation of the controls or cycling of the power to the EUT by the user in accordance with the manufacturer's instructions.

## 8.5. ELECTRICAL FAST TRANSIENT (EFT)

### 8.5.1. TEST SPECIFICATION

|                               |                        |
|-------------------------------|------------------------|
| <b>Basic Standard:</b>        | IEC 61000-4-4          |
| <b>Test Voltage:</b>          | Power Line: $\pm 2$ kV |
| <b>Polarity:</b>              | Positive & Negative    |
| <b>Impulse Frequency:</b>     | 5 kHz                  |
| <b>Impulse Wave-shape:</b>    | 5/50 ns                |
| <b>Burst Duration:</b>        | 15 ms                  |
| <b>Burst Period:</b>          | 300 ms                 |
| <b>Test Duration:</b>         | 2 mins                 |
| <b>Performance Criterion:</b> | B                      |

### 8.5.2. TEST PROCEDURE

EUT is placed on a 0.8 m tall wooden table.

EUT operate at normal mode, the transient/burst was 5/50 ns in accordance with IEC 61000-4-4, both positive and negative polarity burst waveform were applied.

The duration time of each test line was 2 minutes.

### 8.5.3. TEST SETUP

The EUT installed in a representative system as described in section 7 of IEC 61000-4-4.

For the actual test configuration, please refer to the related item – photographs of the test configuration.



#### 8.5.4. TEST RESULT

N/A



## 8.6. SURGE IMMUNITY TEST

### 8.6.1. TEST SPECIFICATION

|                                    |                                                                                               |
|------------------------------------|-----------------------------------------------------------------------------------------------|
| <b>Basic Standard:</b>             | IEC 61000-4-5                                                                                 |
| <b>Wave-Shape:</b>                 | Combination Wave<br>1.2/50 $\mu$ s Open Circuit Voltage<br>8/20 $\mu$ s Short Circuit Current |
| <b>Test Voltage:</b>               | Power Port ~ Line to line: $\pm 1$ kV                                                         |
| <b>Surge Input/Output:</b>         | Power Line: L-N                                                                               |
| <b>Generator Source Impedance:</b> | 2 $\Omega$ between networks<br>12 $\Omega$ between network and ground                         |
| <b>Polarity:</b>                   | Positive/Negative                                                                             |
| <b>Phase Angle:</b>                | 0° /90° /180° /270°                                                                           |
| <b>Pulse Repetition Rate:</b>      | 1 time / min                                                                                  |
| <b>Number of Tests:</b>            | 5 positive polarity pulses, and 5 negative polarity pulses                                    |
| <b>Performance Criterion:</b>      | B                                                                                             |


### 8.6.2. TEST PROCEDURE

EUT is placed on a 0.8 m tall wooden table.

EUT operate at normal mode, two types of combination wave generator (1.2/50 us open-circuit voltage and 8/20 us short-circuit current) are applied to the EUT power supply terminals via the capacitive coupling network.

The power cord between the EUT and the coupling/decoupling network shall not exceed 2 m in length.

### 8.6.3. TEST SETUP

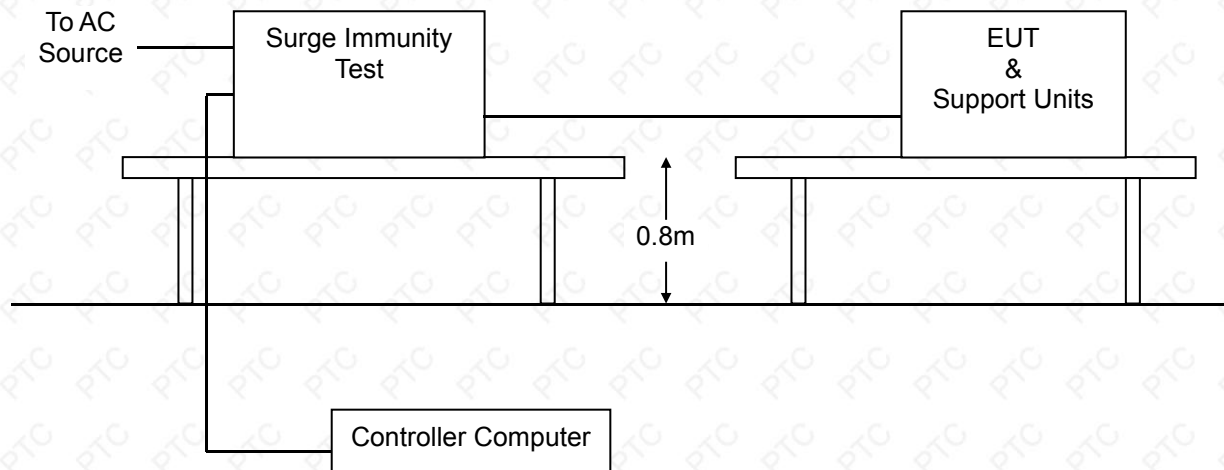

For the actual test configuration, please refer to the related item – Photographs of the Test Configuration.

### 8.6.4. TEST RESULT

N/A

## 8.7. CONDUCTED RADIO FREQUENCY DISTURBANCES (CS)

### 8.7.1. TEST SPECIFICATION

|                               |                                      |
|-------------------------------|--------------------------------------|
| <b>Basic Standard:</b>        | IEC 61000-4-6                        |
| <b>Frequency Range:</b>       | 0.15 MHz ~80 MHz                     |
| <b>Field Strength:</b>        | 3 V                                  |
| <b>Modulation:</b>            | 1 kHz Sine Wave, 80 %, AM Modulation |
| <b>Frequency Step:</b>        | 1 % of preceding frequency value     |
| <b>Coupled cable:</b>         | Power Mains, Shielded                |
| <b>Coupling device:</b>       | CDN-M3/2 (3 wires/2 wires)           |
| <b>Performance Criterion:</b> | A                                    |


### 8.7.2. TEST PROCEDURE

The EUT shall be tested within its intended operating and climatic conditions.

The test shall be performed with the test generator connected to each of the coupling and decoupling devices in turn, while the other non-excited RF input ports of the coupling devices are terminated by a 50  $\Omega$  load resistor.

The frequency range was swept from 150 kHz to 80 MHz, using the signal level established during the setting process and with a disturbance signal of 80 % amplitude. The signal was modulated with a 1 kHz sine wave, pausing to adjust the RF signal level or the switch coupling devices as necessary. The sweep rate was  $1.5 \times 10^{-3}$  decades/s. Where the frequency range is swept incrementally, the step size was 1 % of preceding frequency value the dwell time of the amplitude modulated carrier at each frequency was 0.5 s.

### 8.7.3. TEST SETUP

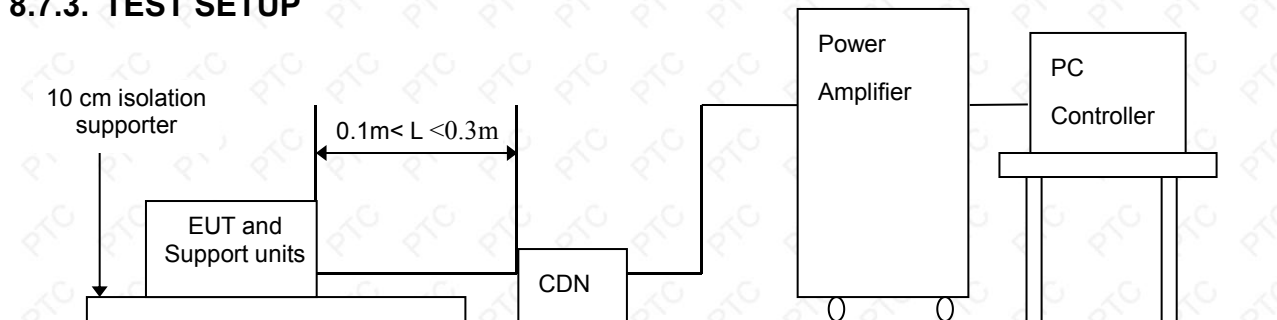

For the actual test configuration, please refer to the related item – Photographs of the Test Configuration

Note: 1) The EUT is setup 0.1 m above Ground Reference Plane

2) All relevant cables shall be provided with the appropriate coupling and decoupling devices at a distance between 0.1 meters and 0.3 meters from the projected geometry of the EUT on the ground reference plane.

### 8.7.4. TEST RESULT

N/A

## 8.8. POWER FREQUENCY MAGNETIC FIELD

### 8.8.1. TEST SPECIFICATION

|                               |                             |
|-------------------------------|-----------------------------|
| <b>Basic Standard:</b>        | IEC 61000-4-8               |
| <b>Frequency Range:</b>       | 50 Hz                       |
| <b>Field Strength:</b>        | 30 A/m                      |
| <b>Observation Time:</b>      | 5 minutes                   |
| <b>Inductance Coil:</b>       | Rectangular type, 1 m x 1 m |
| <b>Performance Criterion:</b> | A                           |

### 8.8.2. TEST PROCEDURE


The equipment is configured and connected to satisfy its functional requirements. It shall be placed on the GRP with the interposition of a 0.1 m-thick insulating support.

The equipment cabinets shall be connected to the safety earth directly on the GRP via the earth terminal of the EUT.

The power supply, input and output circuits shall be connected to the sources of power supply, control and signal.

The cables supplied or recommended by the equipment manufacturer shall be used. 1 meter of all cables used shall be exposed to the magnetic field.

### 8.8.3. TEST SETUP

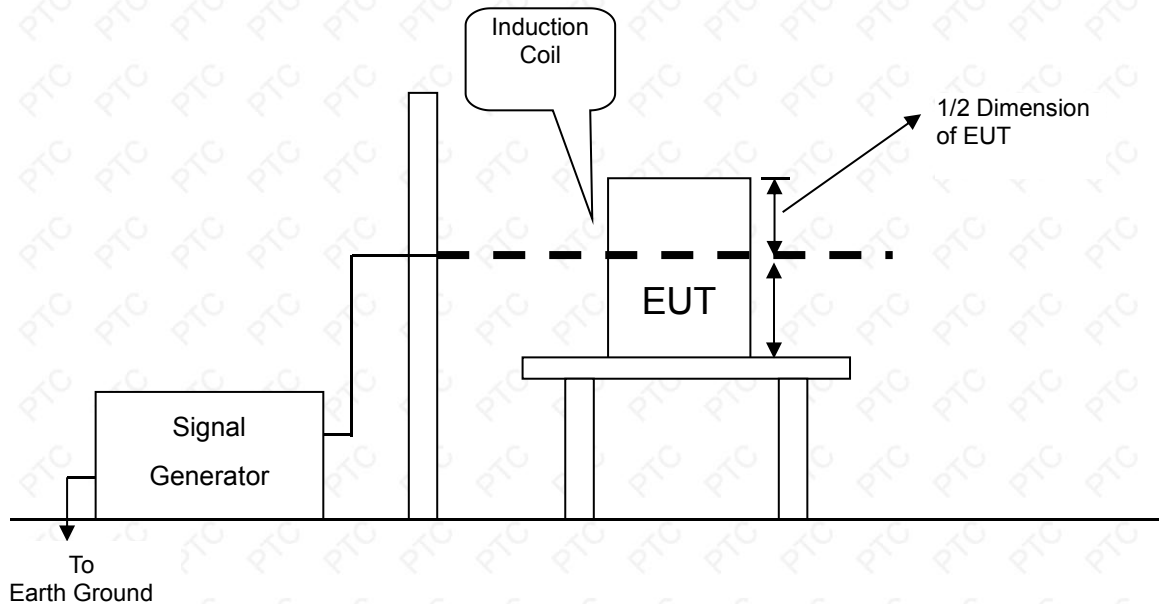

For the actual test configuration, please refer to the related item – Photographs of the Test Configuration  
Note:

#### TABLETOP EQUIPMENT

The equipment shall be subjected to the test magnetic field by using the induction coil of standard dimension (1 m x 1 m). The induction coil shall then be rotated by 90 degrees in order to expose the EUT to the test field with different orientations.

#### FLOOR-STANDING EQUIPMENT

The equipment shall be subjected to the test magnetic field by using induction coils of suitable dimensions. The test shall be repeated by moving and shifting the induction coils, in order to test the whole volume of the EUT for each orthogonal direction. The test shall be repeated with the coil shifted to different positions along the side of the EUT, in steps corresponding to 50 % of the shortest side of the coil. The induction coil shall then be rotated by 90 degrees in order to expose the EUT to the test field with different orientations.

### 8.8.4. TEST RESULT

N/A

## 8.9. VOLTAGE DIP & VOLTAGE INTERRUPTIONS

### 8.9.1. TEST SPECIFICATION

|                                |                                                                                                                                                                                                                                                                         |
|--------------------------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Basic Standard:</b>         | IEC 61000-4-11                                                                                                                                                                                                                                                          |
| <b>Test Duration Time:</b>     | 3 test events in sequence                                                                                                                                                                                                                                               |
| <b>Interval Between Event:</b> | 10 seconds                                                                                                                                                                                                                                                              |
| <b>Phase Angle:</b>            | 0°                                                                                                                                                                                                                                                                      |
| <b>Test Cycle:</b>             | 3 times                                                                                                                                                                                                                                                                 |
| <b>Performance Criterion:</b>  | 0% UT/1 P, Criterion: B<br>40% UT/10 P (For 50Hz), Criterion: C<br>40% UT/12 P (For 60Hz), Criterion: C<br>70% UT/25 P (For 50Hz), Criterion: C<br>70% UT/30 P (For 60Hz), Criterion: C<br>0% UT/250 P (For 50Hz), Criterion: C<br>0% UT/300 P (For 60Hz), Criterion: C |

### 8.9.2. TEST PROCEDURE


The EUT and support units were located on a wooden table, 0.8 m away from ground floor.

Setting the parameter of tests and then perform the test software of test simulator.

Changes to the voltage level shall occur at 0 degree crossing point in the a.c. voltage waveform.

Record the test result in test record form.

### 8.9.3. TEST SETUP

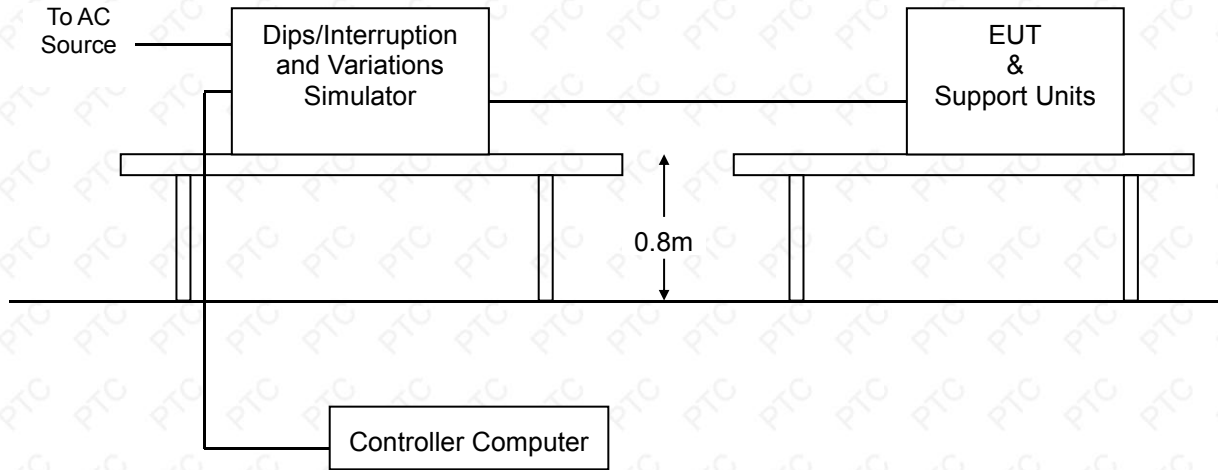

For the actual test configuration, please refer to the related item – Photographs of the Test Configuration.




Report No.: PTC23071004802E-EM01

#### 8.9.4. TEST RESULT


N/A

## 9. PHOTOGRAPHS OF THE TEST CONFIGURATION

### RADIATED EMISSION TEST

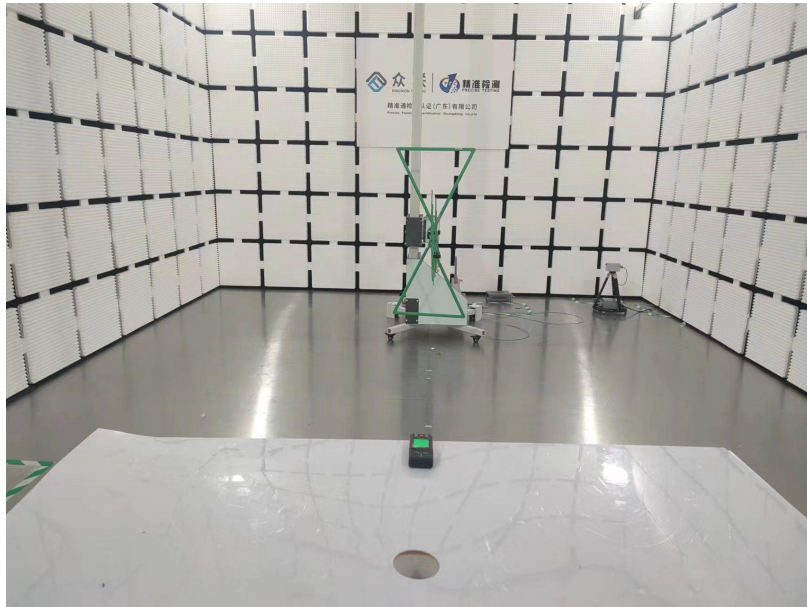

### ESD TEST

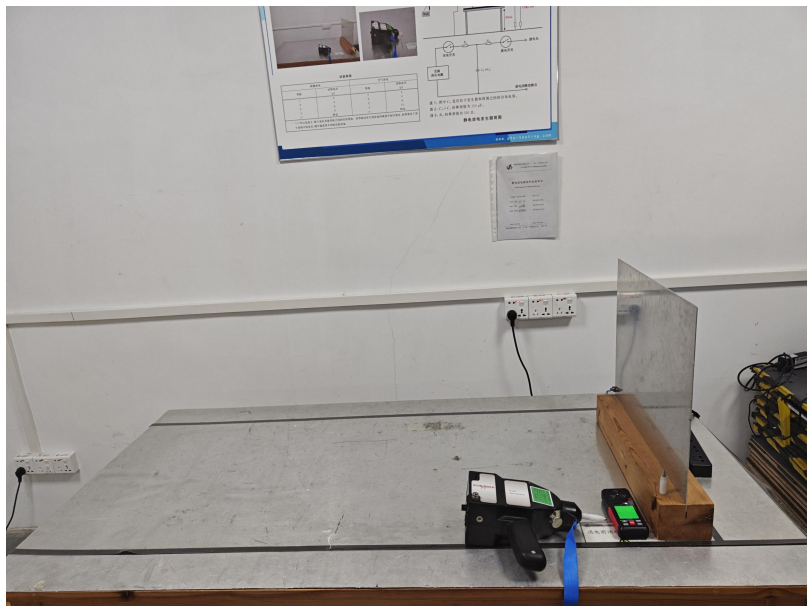

## 10. PHOTOGRAPHS OF EUT







— End of report —